




Melanotan US Inc.  
Leader in Peptide Synthesis

# MS Report GHRP-2

MW: 818.0

## MS Spectrum

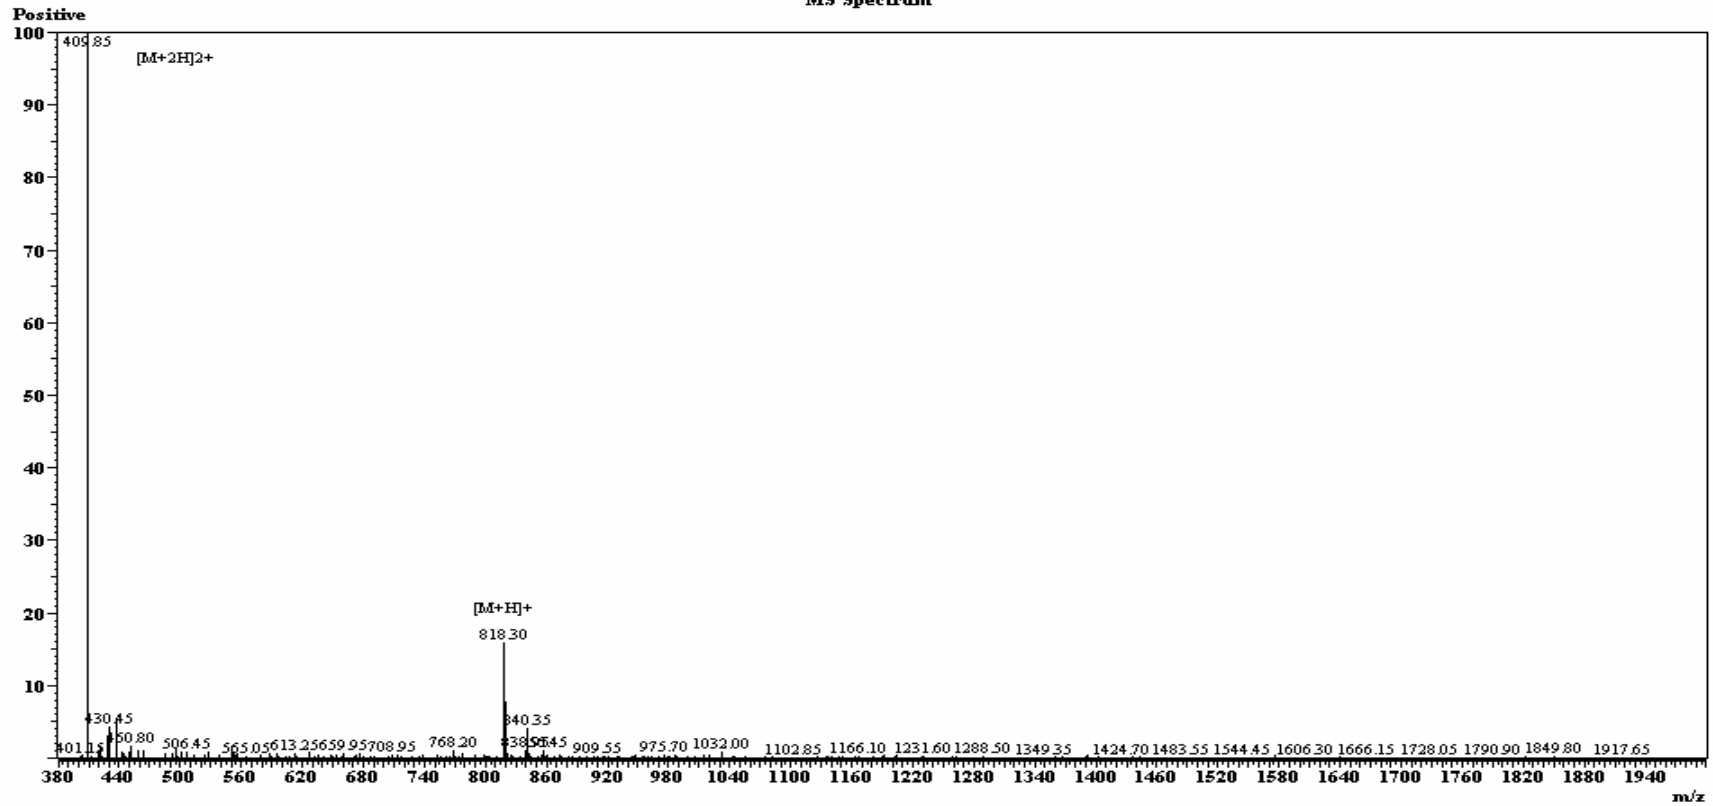

**MS Report**  
**GHRP-2**  
MW: 818.0

**MS conditions:**

Probe:	ESI	Probe bias:	+4.5kv
Nebulizer Gas Flow:	1.5L/min	Detector:	1.5kv
CDL:	-20.0v	T. Flow:	0.2ml/min
CDL Temp:	250°C	B. conc:	50%H2O/50%ACN
Block Temp:	200°C		